SOURCE OF STERILANT 10 WITHOUT LUMEN DEVICE ACROSS TWO CHAMBERS 12 VACUUM PUMP PUMP 18 16 150 SOURCE OF STERILANT

(THE TWO ENCLOSURES FOR THE SOURCE OF PEROXIDE CAN BE COMBINED AS ONE)

FIG. 1A



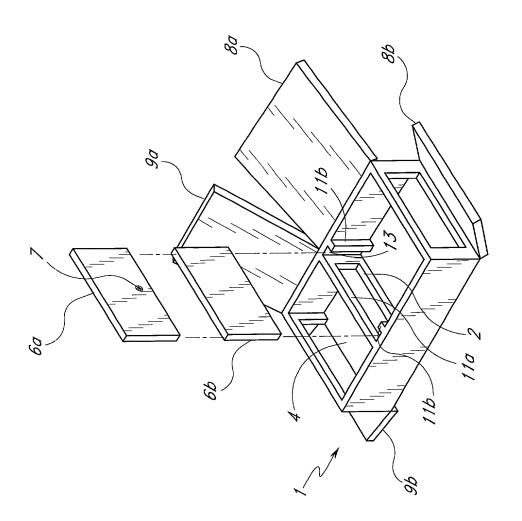


FIG. 1B

m

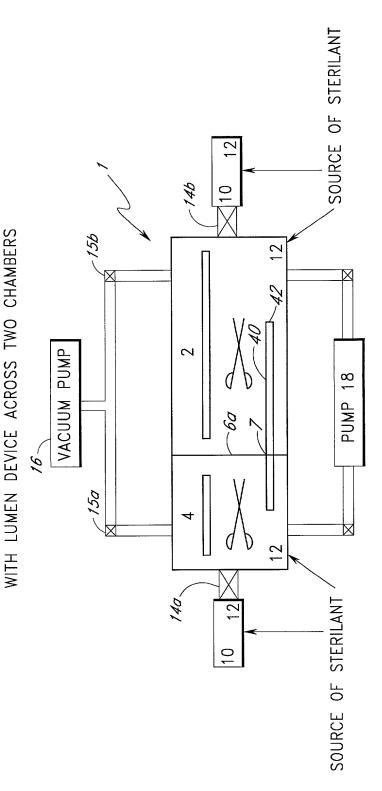

(THE TWO ENCLOSURES FOR THE SOURCE OF PEROXIDE CAN BE COMBINED AS ONE)

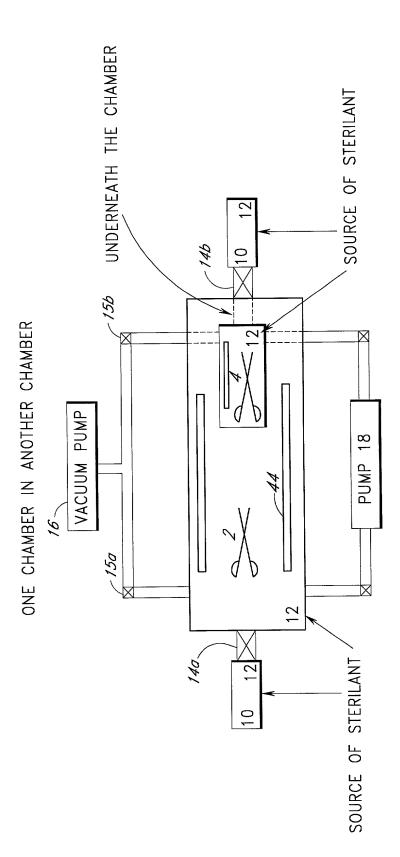

(THE TWO ENCLOSURES FOR THE SOURCE OF PEROXIDE CAN BE COMBINED AS ONE)


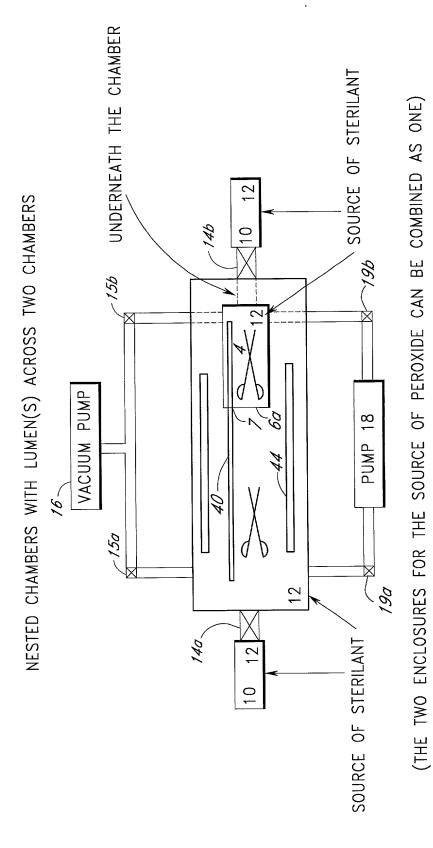



FIG.4

THE USE OF CONTAINER IN THE SYSTEM-CONFIGURATION 1

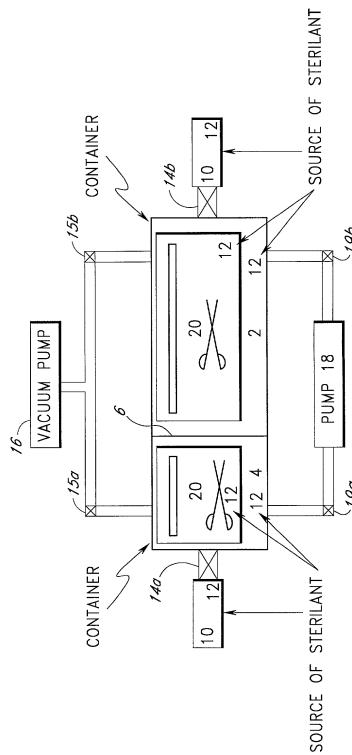

(THE TWO ENCLOSURES FOR THE SOURCE OF PEROXIDE CAN BE COMBINED AS ONE)

THE USE OF CONTAINER IN THE SYSTEM-CONFIGURATION 2

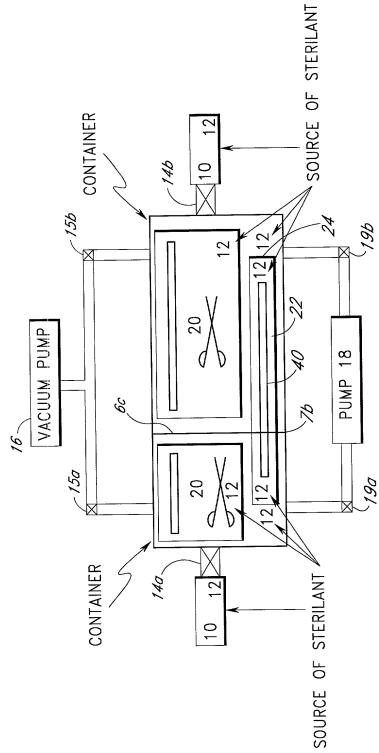

(THE TWO ENCLOSURES FOR THE SOURCE OF PEROXIDE CAN BE COMBINED AS ONE)









FIG.6B

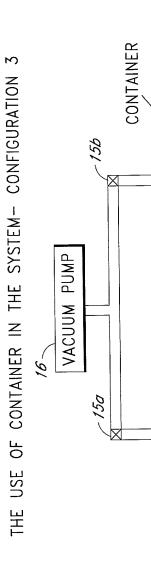


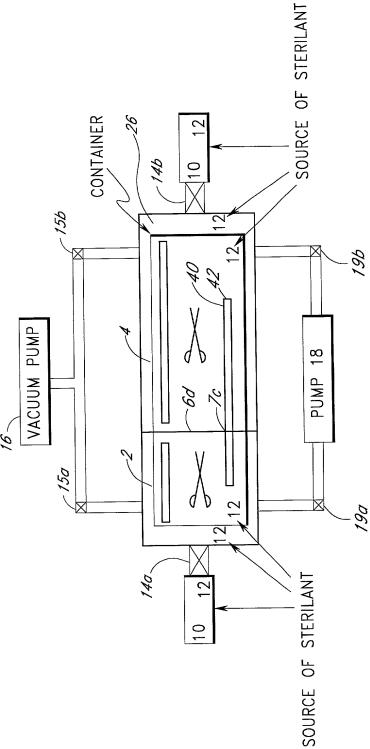


(THE TWO ENCLOSURES FOR THE SOURCE OF PEROXIDE CAN BE COMBINED AS ONE)

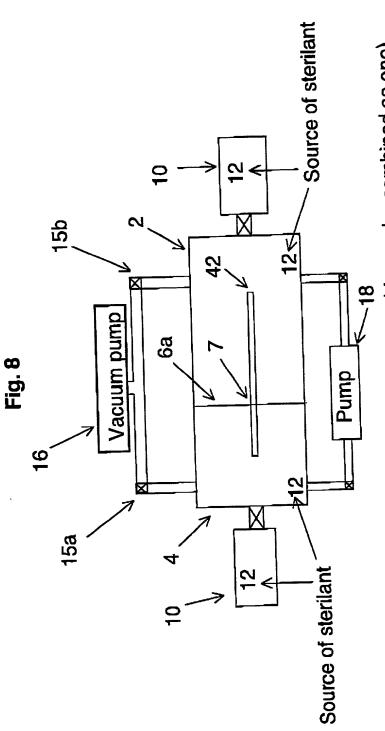

(These two enclosures for the source of peroxide can be combined as one)

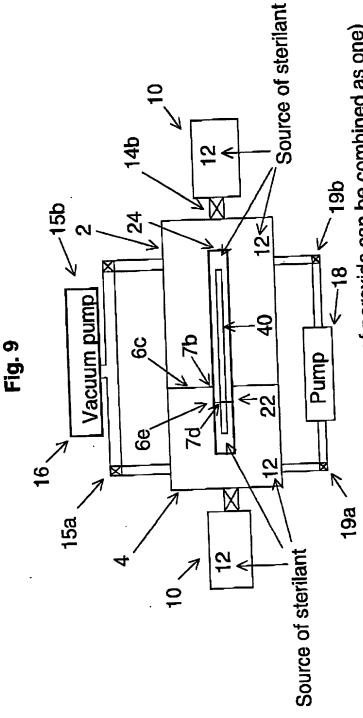

(These two enclosures for the source of peroxide can be combined as one)

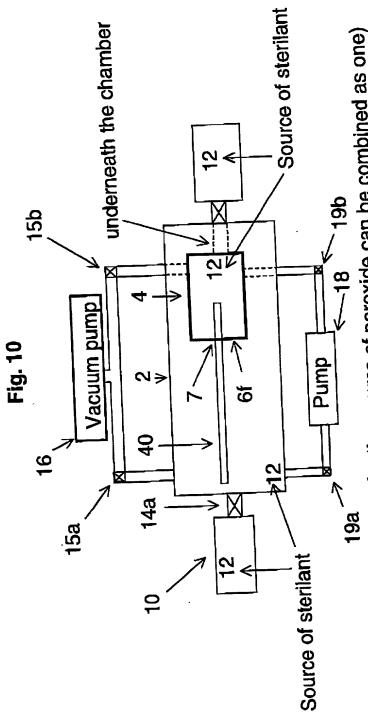

(These two enclosures for the source of peroxide can be combined as one)

